

# ELISA Kit for Cutaneous T-Cell Attracting Chemokine (CTACK)

Catalog No: tcue862



## Available Sizes

Size: 96T



## Specifications

### Research Area:

Cytokine;Tumor immunity;Infection immunity;Dermatology;

### Species Reactivity:

Homo sapiens (Human)

### Sample Type:

serum, plasma, tissue homogenates, cell lysates, cell culture supernates and other biological fluids

### Sensitivity:

The minimum detectable dose of this kit is typically less than 12.9pg/mL

### Detection Range:

31.2-2,000pg/mL

### Assay Time:

3h

### Detection Method:

Enzyme-linked immunosorbent assay for Antigen Detection.

### Tested Application:


ELISA

### SwissProt:

Q9Y4X3

## Test Principle

The test principle applied in this kit is Sandwich enzyme immunoassay. The microtiter plate provided in this kit has been pre-coated with an antibody specific to Cutaneous T-Cell Attracting Chemokine (CTACK). Standards or samples are then added to the appropriate microtiter plate wells with a biotin-conjugated antibody specific to Cutaneous T-Cell Attracting Chemokine (CTACK). Next, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. After TMB substrate solution is added, only those wells that contain Cutaneous T-Cell Attracting Chemokine (CTACK), biotin-conjugated antibody and enzyme-conjugated Avidin will exhibit a change in color. The enzyme-substrate reaction is terminated by the addition of sulphuric acid solution and the color change is measured spectrophotometrically at a wavelength of  $450\text{nm} \pm 10\text{nm}$ . The concentration of Cutaneous T-Cell Attracting Chemokine (CTACK) in the samples is then determined by comparing the O.D. of the samples to the standard curve.

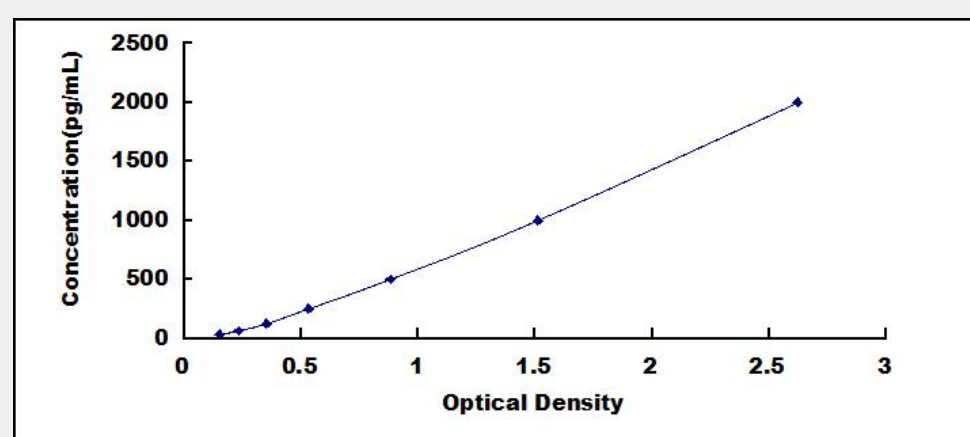

All products are for RESEARCH USE ONLY. Not for diagnostic & therapeutic purposes!